



**More Than 6 Million Times**  
Around the world, MEDRAD® Intego  
has been trusted for PET infusions.  
A Smart Choice!

## The Protector by Your Side

**Fully automated dose preparation  
and patient infusion in a single,  
easy-to-use, mobile system\* to:**

- Reduce clinicians radiation exposure
- Deliver patient dose accuracy
- Personalize patient care
- Drive operational efficiency

**MEDRAD® Intego**  
PET Infusion System


\* PET Infusion System for the dose administration/delivery of 18F-FDG or 18F-NaF

More than 6 Million

6,000,000

**Worldwide Infusions\***  
**Cumulative with MEDRAD® Intego.**  
**And Counting.**

Worldwide cumulative infusions  
with MEDRAD® Intego  
(August 2008 – May 2022)

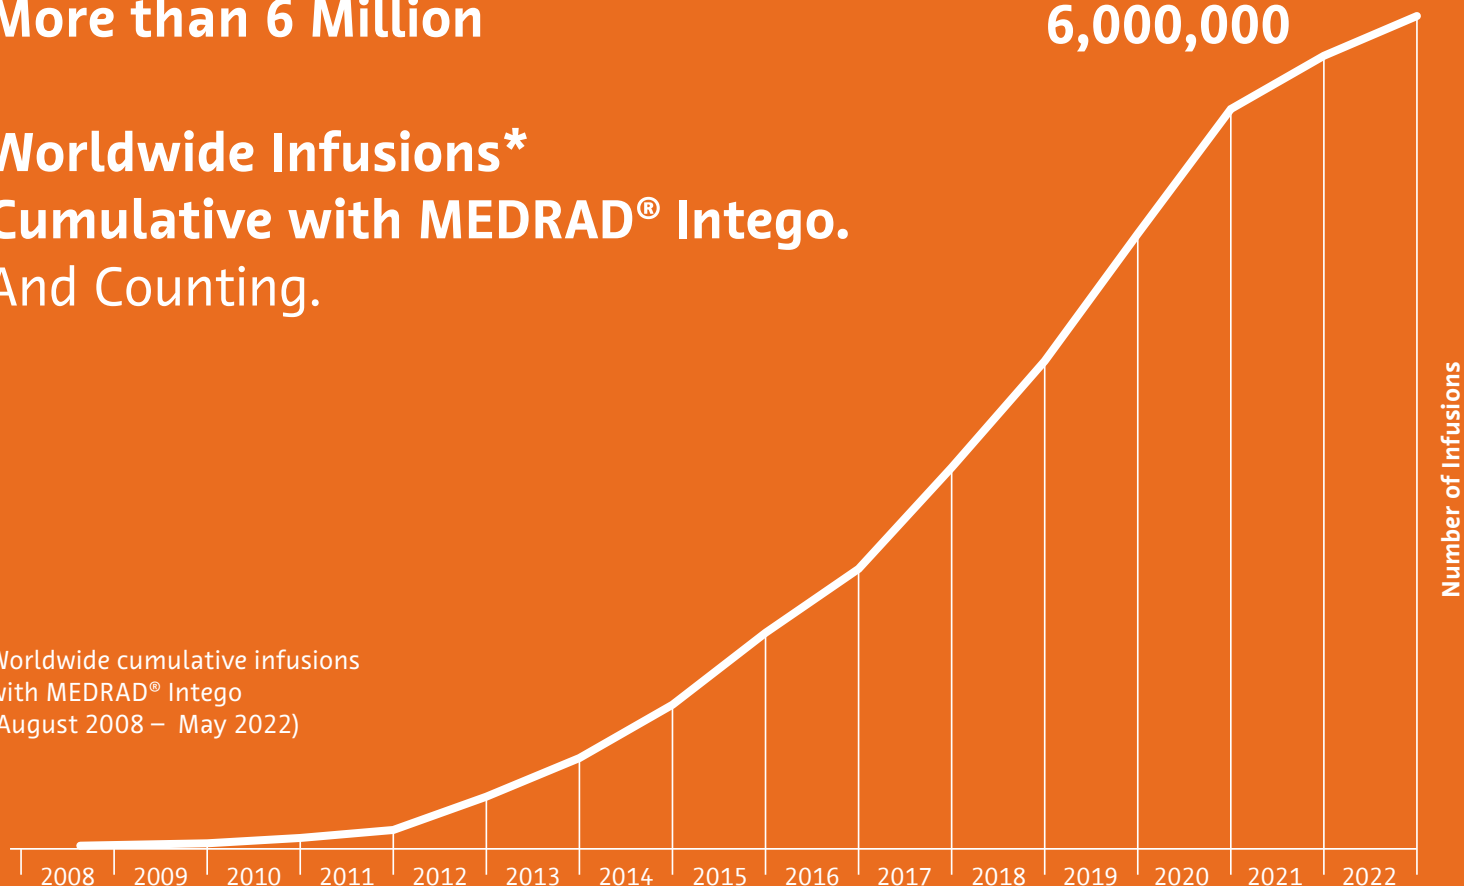

**One PET infusion is done every 26 seconds\*\***  
**with MEDRAD® Intego.**

Based on Worldwide Patient Administration Set sales data August 2008 – May 2022.

\*\* Based on Worldwide Patient Administration Set sales in 2021 and 250 working days/year.

**Clear Direction. > From Diagnosis to Care.**

Bayer reserves the right to modify the specifications and features described herein or to discontinue any product or service identified in this publication at any time without prior notice or obligation. Please contact your authorized Bayer representative for the most current information.

All patient data that appear in this document are fictitious. No actual patient information is shown.

Bayer, the Bayer Cross, MEDRAD and MEDRAD Intego are trademarks owned by and/or registered to Bayer in the U.S. and/or other countries. Other trademarks and company names mentioned herein are properties of their respective owners and are used herein solely for informational purposes. No relationship or endorsement should be inferred or implied.

INT001E © 2022 Bayer. This material may not be reproduced, displayed, modified or distributed without the express prior written consent of Bayer.



Bayer Inc.  
2920 Matheson Blvd East,  
Mississauga (Ontario) L4W 5R6  
Telephone: 800-268-1432  
Fax machine: 800-567-1710

CE 2797

PP-PF-RAD-CA-0605-1 July 2022